


DORO Aluminium Head Rest System

DORO Aluminium Head Rest System for supine, prone, lateral and sitting position (for sitting position Crossbar Adaptor is required). Excellent stability and flexibility. 3-pin rigid cranial fixation. Cannot be used for any MRI Imaging. Fixing Adaptor 60146 required for Promerix and Practico

Includes the items below:

101 001 001 *Doro QR3 Skull Clamp*
100 300 200 *Doro Swivel Adaptor Aluminium*
100 300 100 *Doro Base Unit Aluminium*

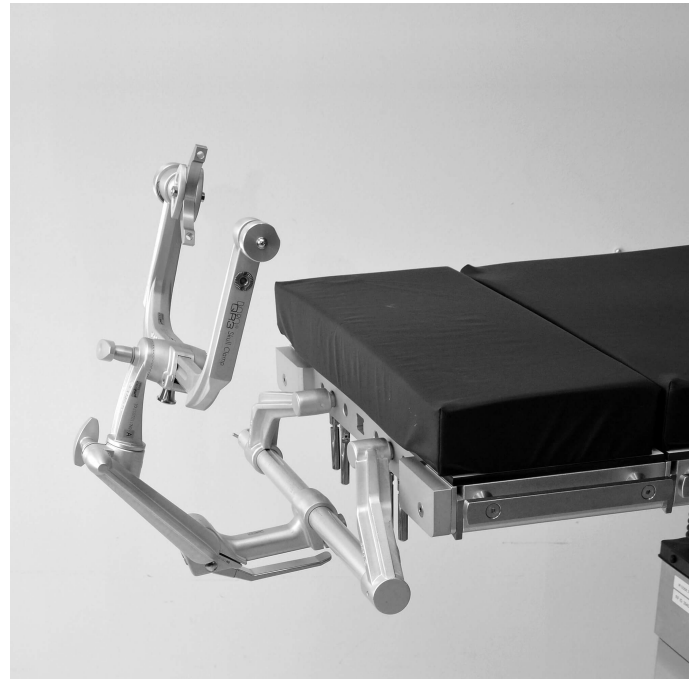

Technical Specifications

Product Code	101001100
--------------	-----------

Ota yhteyttä

Merivaara Corp.
Tarmontie 2-4
15860 HOLLOLA
SUOMI

+358 3 3394 611

merivaara@merivaara.com

